

## PRODUCT DATA SHEET

Standing: 2021-06-01

### LAUDA PRO RP 250 E

Cooling heating circulator 230 V; 50 Hz

Part Number: L002494

#### Features

- Thermostatic circulator with latest microprocessor technology. Integrated cooling system
- Bright and high-contrast graphic OLED display
- Integrated programmer, 1 programme with max. 20 segments
- Operation with Cursor- and Softkeys
- EasyUse system for simple operation of the whole unit
- SelfCheck Assistant for system diagnosis
- Command console can be detached and used as remote control
- Tower design with small footprint
- Low filling volume enables rapid changes in temperature
- Bath vessel made of stainless steel (insulated, with overflow and drain tap)
- LAUDA Varioflex pump (pressure/suction) with 8 selectable levels, connections rear
- USB and Ethernet interface equipped as standard
- Retrofittable for upgrading with interface (RS 232/485, Profibus; EtherCAT; analogue or contact modules)
- Fully electronic continuous controller with PID action for internal & external control
- PowerAdapt system for the use of the maximum possible amount of heat permitted by the power supply system
- Low-level and adjustable over-temperature protection with acoustic alarm for use with flammable and non-flammable liquids
- SmartCool system for energy-saving digital cooling management including compressor on-off control
- Hybrid cooling system: (heat removal complementary with cooling water)
- Utilizes natural refrigerants



Reserve technical changes



Working temperature min.  
-50 °C



Working temperature max.  
200 °C

LAUDA DR. R. WOBSEY GMBH & CO. KG  
Pfarrstraße 41/43 • 97922 Lauda-Königshofen  
Postfach 1251 • 97912 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0 • F + 49 (0) 9343 503-222  
info@lauda.de • www.lauda.de  
WEEE-Reg-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
Registergericht Mannheim • HRA 560069

Persönlich haftende Gesellschafterin:  
LAUDA DR. R. WOBSEY Verwaltungs-GmbH  
Sitz Lauda-Königshofen  
Registergericht Mannheim • HRB 560226

Geschäftsführer:  
Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
Dr. Marc Stricker  
Beirat: Dr. Gerhard Wobser

## PRODUCT DATA SHEET

Standing: 2021-06-01

LAUDA PRO RP 250 E

Cooling heating circulator 230 V; 50 Hz

Part Number: L002494

### Technical Features

Working temperature range	-50 ... 200 °C
Operating temperature range	-50 ... 200 °C
Ambient temperature range	5 ... 40 °C
Temperature stability	0.05 ± K
Heater power max.	2.5 kW
Power consumption max.	3.7 kW
Power consumption	16 A
Pump Pressure max.	0.7 bar
Pump flow rate pressure max.	22 L/min
In / Outlet connection thread (outside)	M16x1
In / Outlet Ø olives	13 mm
Filling volume min.	2.4 L
Filling volume max.	4.4 L
Overall dimensions (WxDxH)	300 x 430 x 675 mm
Refrigerant stage 1	R-290 (GWP 3); 0.140 kg; 0.0 t CO <sub>2</sub> -eq
Power supply	230 V; 50 Hz
Power plug	Power cord with angled plug (CEE7/7)

Reserve technical changes

LAUDA DR. R. WOBSEY GMBH & CO. KG  
Pfarrstraße 41/43 • 97922 Lauda-Königshofen  
Postfach 1251 • 97912 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0 • F + 49 (0) 9343 503-222  
info@lauda.de • www.lauda.de  
WEEE-Reg-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
Registergericht Mannheim • HRA 560069

Persönlich haftende Gesellschafterin:  
LAUDA DR. R. WOBSEY Verwaltungs-GmbH  
Sitz Lauda-Königshofen  
Registergericht Mannheim • HRB 560226

Geschäftsführer:  
Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
Dr. Marc Stricker  
Beirat: Dr. Gerhard Wobser

## PRODUCT DATA SHEET

Standing: 2021-06-01

LAUDA PRO RP 250 E

Cooling heating circulator 230 V; 50 Hz

Part Number: L002494

Temperature	Pump stage	Heat transfer liquid	Cooling Capacity 50 Hz
20 °C	8	Ethanol	1.5 kW
10 °C	8	Ethanol	1.44 kW
0 °C	8	Ethanol	1.2 kW
-10 °C	8	Ethanol	0.84 kW
-20 °C	4	Ethanol	0.54 kW
-30 °C	4	Ethanol	0.29 kW
-40 °C	4	Ethanol	0.11 kW
-45 °C	4	Ethanol	0.04 kW
-50 °C	2	Ethanol	0.02 kW

### Standard accessories

- 2 screw caps, 2 closing plugs
- 2 nipples 13 mm for pump connectors
- 2 nipples 10 mm with screw cap G3/8 for cooling water

LAUDA DR. R. WOBSEY GMBH & CO. KG  
Pfarrstraße 41/43 • 97922 Lauda-Königshofen  
Postfach 1251 • 97912 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0 • F + 49 (0) 9343 503-222  
info@lauda.de • www.lauda.de  
WEEE-Reg-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
Registergericht Mannheim • HRA 560069

Persönlich haftende Gesellschafterin:  
LAUDA DR. R. WOBSEY Verwaltungs-GmbH  
Sitz Lauda-Königshofen  
Registergericht Mannheim • HRB 560226

Geschäftsführer:  
Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
Dr. Marc Stricker  
Beirat: Dr. Gerhard Wobser


## PRODUCT DATA SHEET

Standing: 2021-06-01

LAUDA PRO RP 250 E

Cooling heating circulator 230 V; 50 Hz

Part Number: L002494

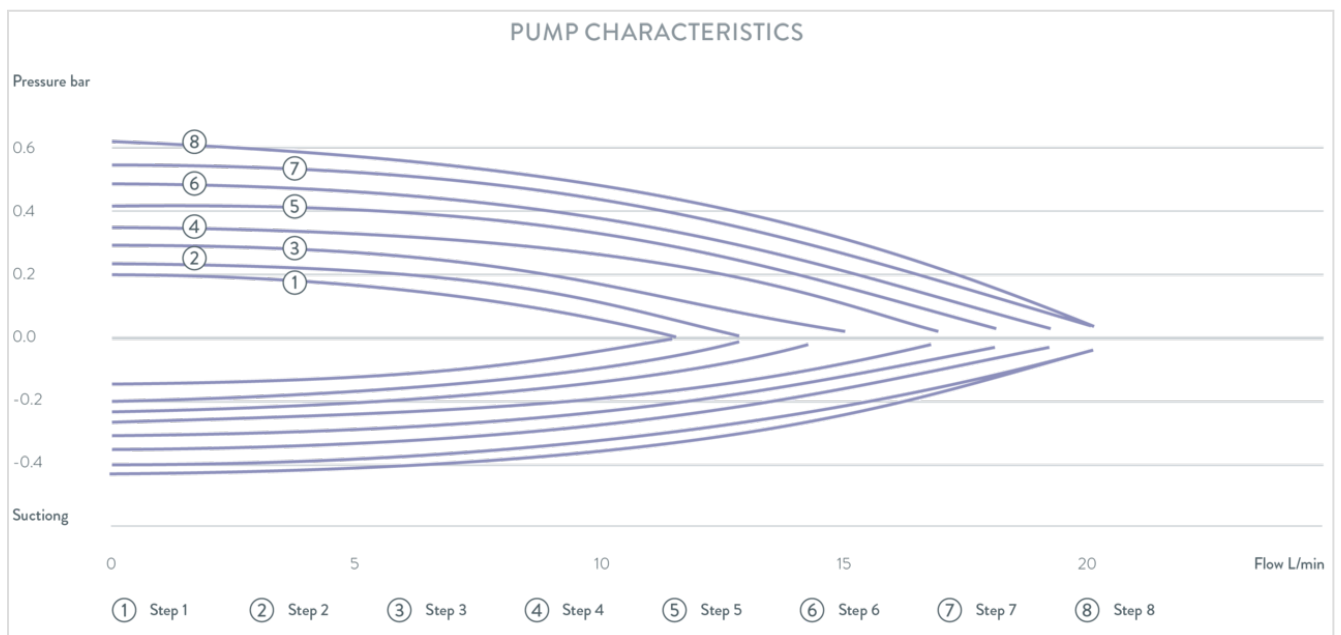

Reserve technical changes

LAUDA DR. R. WOBSEY GMBH & CO. KG  
Pfarrstraße 41/43 • 97922 Lauda-Königshofen  
Postfach 1251 • 97912 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0 • F + 49 (0) 9343 503-222  
info@lauda.de • www.lauda.de  
WEEE-Reg-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
Registergericht Mannheim • HRA 560069

Persönlich haftende Gesellschafterin:  
LAUDA DR. R. WOBSEY Verwaltungs-GmbH  
Sitz Lauda-Königshofen  
Registergericht Mannheim • HRB 560226

Geschäftsführer:  
Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
Dr. Marc Stricker  
Beirat: Dr. Gerhard Wobser