

## PRODUCT DATA SHEET

Published: 2026-06-22

LAUDA Ultratemp UT 3505 W Process thermostat  
400 V; 3/PE; 50 Hz & 460 V; 3/PE; 60 Hz  
Part Number: L004025

### Features

- Process thermostat with integrated heater
- Graphic LCD with clear text menu navigation
- Operation possible via web server
- Integrated Ethernet interface
- Connection external Pt100 temperature sensor
- Fully electronic continuous controller with PID action
- Protection level IP 54 (for outdoor installation)
- Stainless steel housing
- Industrial block pump with high pressure and high flow rate
- Additional pump for internal circulation
- Digital display of pump pressure
- Operates with non flammable liquids (water, water/glycol)
- Integrated water filter
- Utilises traditional refrigerants (HFCs) in accordance with European legislation to control F-gases (EU) 573/2024
- Condenser cooling Water
- Certification according to UL 60335:2023, CSA 22.2 No. 60335 Ed. 2nd



Reserve technical changes



Working temperature min.  
-5 °C



Working temperature max.  
60 °C

LAUDA DR. R. WOBSEY GMBH & CO. KG  
Laudaplatz 1 • 97922 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0  
info@lauda.de • www.lauda.de  
WEEE-Reg.-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
Registergericht Mannheim • HRA 560069

Persönlich haftende Gesellschafterin:  
LAUDA DR. R. WOBSEY Verwaltungs-GmbH  
Sitz Lauda-Königshofen  
Registergericht Mannheim • HRB 560226

Geschäftsführer:  
Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
Dr. Marc Stricker  
Beirat: Dr. Gerhard Wobser

# PRODUCT DATA SHEET

Published: 2026-06-22

LAUDA Ultratemp UT 3505 W Process thermostat  
 400 V; 3/PE; 50 Hz & 460 V; 3/PE; 60 Hz  
 Part Number: L004025

## Technical Features

Working temperature range	-5 ... 60 °C
Ambient temperature range	-15 ... 50 °C
Temperature stability	0.5 ± K
Heater power max.	35 kW
Pump Pressure max. 50 Hz	3.2 bar
Pump pressure nominal 50 Hz	3 bar
Flow rate max. (pressure) 50 Hz	250 L/min
Pump pressure max. 60 Hz	4.6 bar
Flow rate max. (pressure) 60 Hz	300 L/min
Pump pressure nominal 60 Hz	4.4 bar
Pump flow rate nominal	90 L/min
In / Outlet connection thread (inside)	Rp 11/2
Water cooling connection thread (inside)	Rp 11/2
Filling volume max.	100 L
Cooling water temperature min.	0 °C
Cooling water temperature max.	45 °C
Pressure difference cooling water min.	2 bar
Maximum pressure cooling water	6 bar
Cooling water consumption	82.9 L/min
Refrigerant stage 1	R-407C (GWP 1770); 3.200 kg; 5.7 t CO <sub>2</sub> -eq
Protection rating	IP 54
Overall dimensions (WxDxH)	1138 x 1486 x 1792 mm
Weight	585 kg
Power plug	---
Power supply	400 V; 3/PE; 50 Hz & 460 V; 3/PE; 60 Hz
Current max.	80 A

Reserve technical changes

LAUDA DR. R. WOBSEER GMBH & CO. KG  
 Laudaplatz 1 • 97922 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0  
 info@lauda.de • www.lauda.de  
 WEEE-Reg.-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
 Registergericht Mannheim • HRA 560069

Persönlich haftende Gesellschafterin:  
 LAUDA DR. R. WOBSEER Verwaltungs-GmbH  
 Sitz Lauda-Königshofen  
 Registergericht Mannheim • HRB 560226

Geschäftsführer:  
 Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
 Dr. Marc Stricker  
 Beirat: Dr. Gerhard Wobser

## PRODUCT DATA SHEET

Published: 2026-06-22

LAUDA Ultratemp UT 3505 W Process thermostat  
400 V; 3/PE; 50 Hz & 460 V; 3/PE; 60 Hz  
Part Number: L004025

Temperature	Cooling Capacity 50 Hz	Cooling Capacity 60 Hz
60 °C	39.2 kW	45.8 kW
30 °C	39.2 kW	45.8 kW
20 °C	35.3 kW	41.1 kW
15 °C	30.5 kW	35.5 kW
10 °C	26.2 kW	29.4 kW
5 °C	22 kW	25.6 kW
0 °C	18.7 kW	21.7 kW
-5 °C	15.1 kW	17.5 kW

Reserve technical changes

LAUDA DR. R. WOBSEY GMBH & CO. KG  
Laudaplatz 1 • 97922 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0  
info@lauda.de • www.lauda.de  
WEEE-Reg.-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
Registergericht Mannheim • HRA 560069


Persönlich haftende Gesellschafterin:  
LAUDA DR. R. WOBSEY Verwaltungs-GmbH  
Sitz Lauda-Königshofen  
Registergericht Mannheim • HRB 560226

Geschäftsführer:  
Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
Dr. Marc Stricker  
Beirat: Dr. Gerhard Wobser

## PRODUCT DATA SHEET

Published: 2026-06-22

LAUDA Ultratemp UT 3505 W Process thermostat  
 400 V; 3/PE; 50 Hz & 460 V; 3/PE; 60 Hz  
 Part Number: L004025

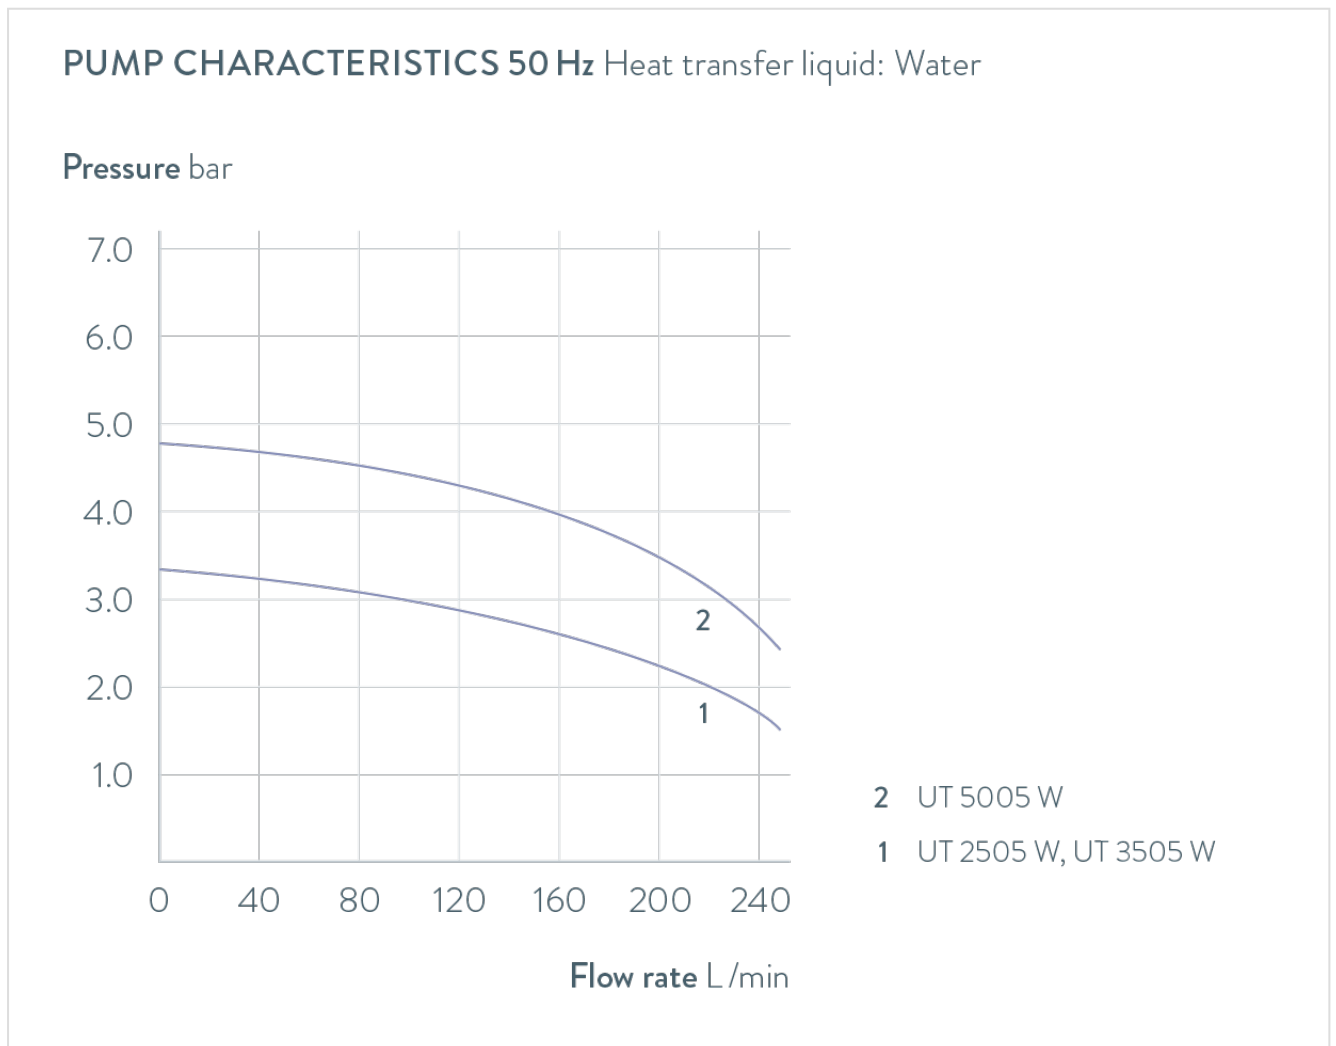

Reserve technical changes

LAUDA DR. R. WOBSEY GMBH & CO. KG  
 Laudaplatz 1 • 97922 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0  
 info@lauda.de • www.lauda.de  
 WEEE-Reg-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
 Registergericht Mannheim • HRA 560069


Persönlich haftende Gesellschafterin:  
 LAUDA DR. R. WOBSEY Verwaltungs-GmbH  
 Sitz Lauda-Königshofen  
 Registergericht Mannheim • HRB 560226

Geschäftsführer:  
 Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
 Dr. Marc Stricker  
 Beirat: Dr. Gerhard Wobser

## PRODUCT DATA SHEET

Published: 2026-06-22

LAUDA Ultratemp UT 3505 W Process thermostat  
400 V; 3/PE; 50 Hz & 460 V; 3/PE; 60 Hz  
Part Number: L004025

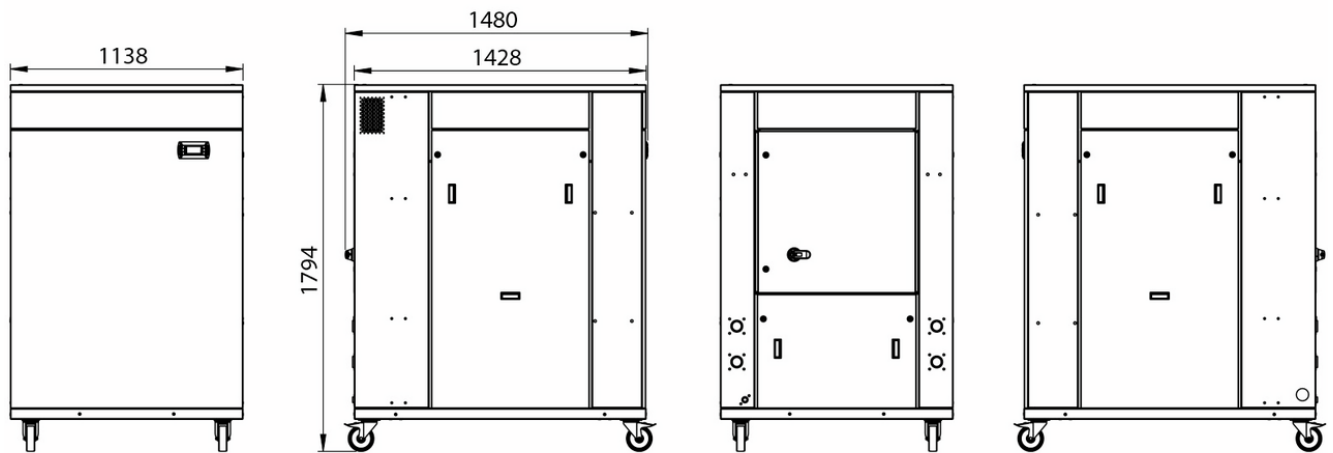

Reserve technical changes

LAUDA DR. R. WOBSEY GMBH & CO. KG  
Laudaplatz 1 • 97922 Lauda-Königshofen • DE

T + 49 (0) 9343 503-0  
info@lauda.de • www.lauda.de  
WEEE-Reg.-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen  
Registergericht Mannheim • HRA 560069

Persönlich haftende Gesellschafterin:  
LAUDA DR. R. WOBSEY Verwaltungs-GmbH  
Sitz Lauda-Königshofen  
Registergericht Mannheim • HRB 560226

Geschäftsführer:  
Dr. Gunther Wobser (Vors.), Dr. Mario Englert,  
Dr. Marc Stricker  
Beirat: Dr. Gerhard Wobser